

Scan-Field Calibration Report

Machine Serial Number : S0711Q0147

Operator : TITA500fr

Calibration date : 2026-01-26

RESULTS


Average Error ($\leq 30 \mu\text{m}$) : $14 \mu\text{m}$

Max Error ($\leq 60 \mu\text{m}$) : $31 \mu\text{m}$



Pass

Previous Scan-Head Error

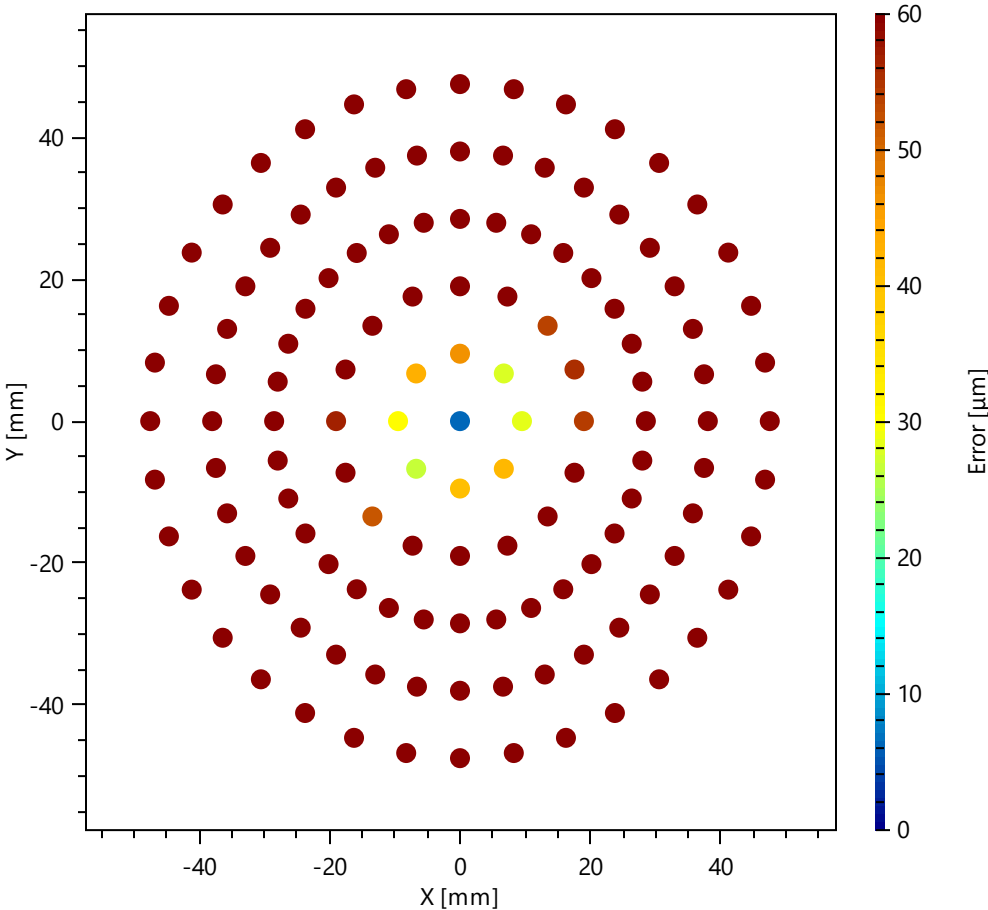

Current Scan-Head Error

